
## **Response by iPS-Derived Hepatocytes to Negative Control Compounds**

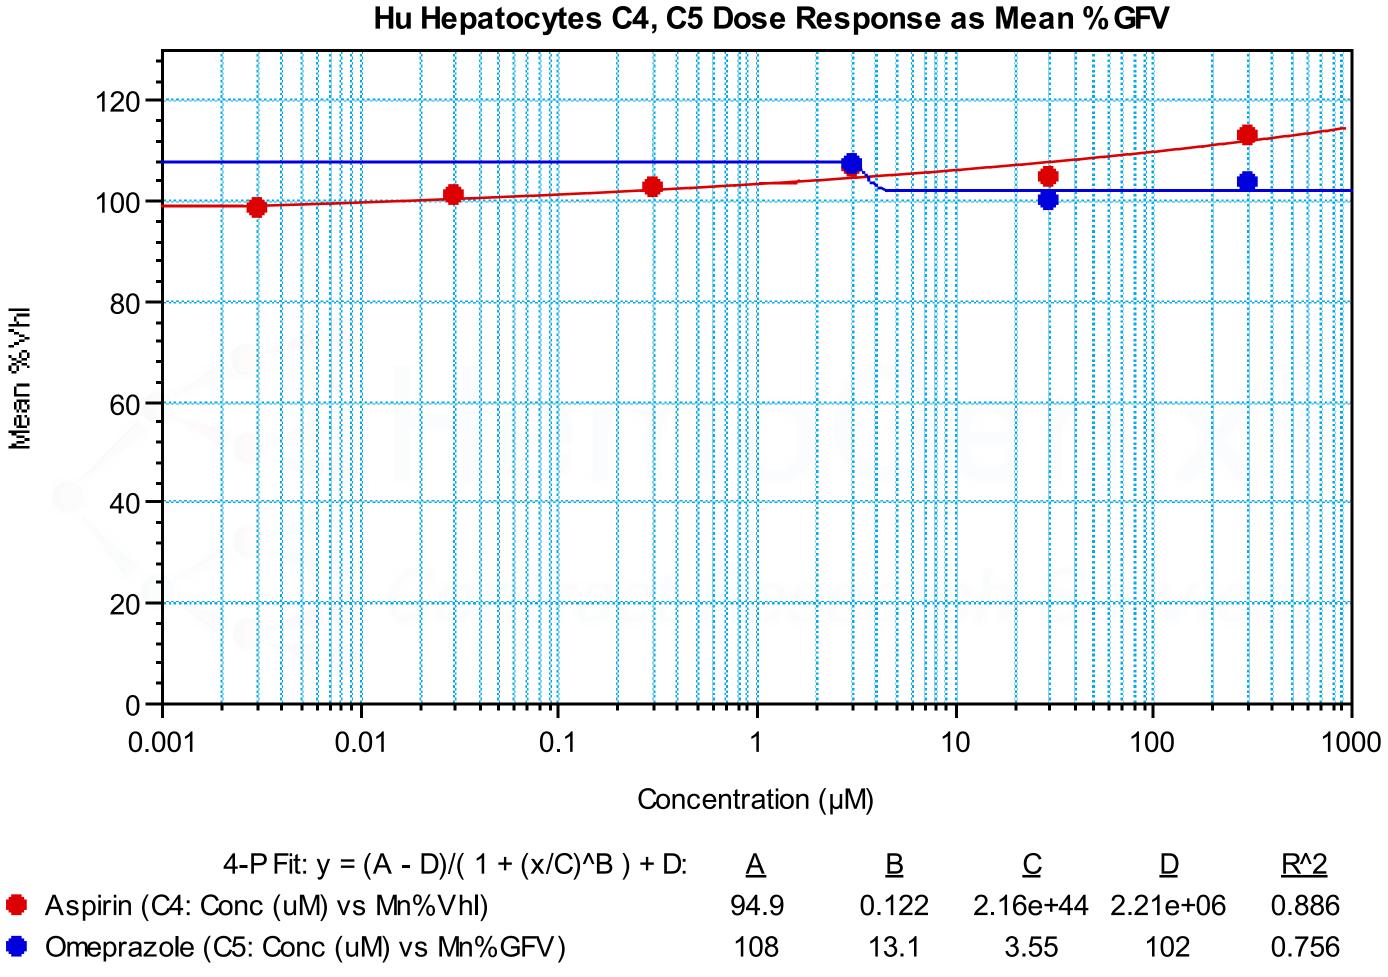

Weighting: Fixed

Mean %Vhl

Results shown are those obtained using SoftMax Pro Software from Molecular Devices